



**Mission Mountain Laboratories. Inc.**

82892 US Hwy 93  
Ravalli, MT 59863  
Phone: 406-726-5227  
www.mml-labs.com



Accredited to ISO/IEC 17025:2017  
Accreditation #86228

## Certificate of Analysis

**Canyonside Labs**  
621 Washington St South  
Suite 700  
Twin Falls, ID  
83301

**Order ID:** 2201133506  
**Lab Sample #:** 43713639  
**Receive Date:** 01/13/2022 01:11PM  
**Report ID:** #9904

**Sample Description:** Luteolin

**Receive Condition:** Good  
**Sample Lot #:** 11083/2022005 **Storage Condition:** Ambient

<b>Identity</b>	<b>Result</b>	<b>Specification</b>	<b>Analyst</b>	<b>Date</b>	<b>Method</b>
*FTIR	Conforms	Conforms	Allista Vetter	01/18/2022	MML220.02

### Method References

**Method #** MML220.02 **Desc** Identification by FTIR  
**Instrument** FTIR

### Approval

**Approved By:**

Kimberly Nuccio  
President/Authorized Reviewer

**Approved Date:** 01/19/2022

**Laboratory Location:** 82892 US Hwy 93 N, Ravalli, MT 59863

Disclaimer: This product results are only applicable to test sample submitted. Mission Mountain Laboratory makes no claims as to the efficacy, safety, or other risks associated with any detected or non-detected levels of any compounds reported herein. This certificate shall not be reproduced except in full, without the written approval of Mission Mountain Laboratories. Quality and uncertainty data is available upon request. Testing listed above may not be included in our current PJLA scope of accreditation. Please consult PJLA Certificate# 86228 for a list of current accredited tests.




# FTIR Report

## Report Details

Report Location C:\pel\_data\templates\standard\MML 43713639 Luteolin Canyonside UATR  
Report Creator Allista Vetter  
Report Date 18 January, 2022 10:47

## Compare Results

### Result Spectrum

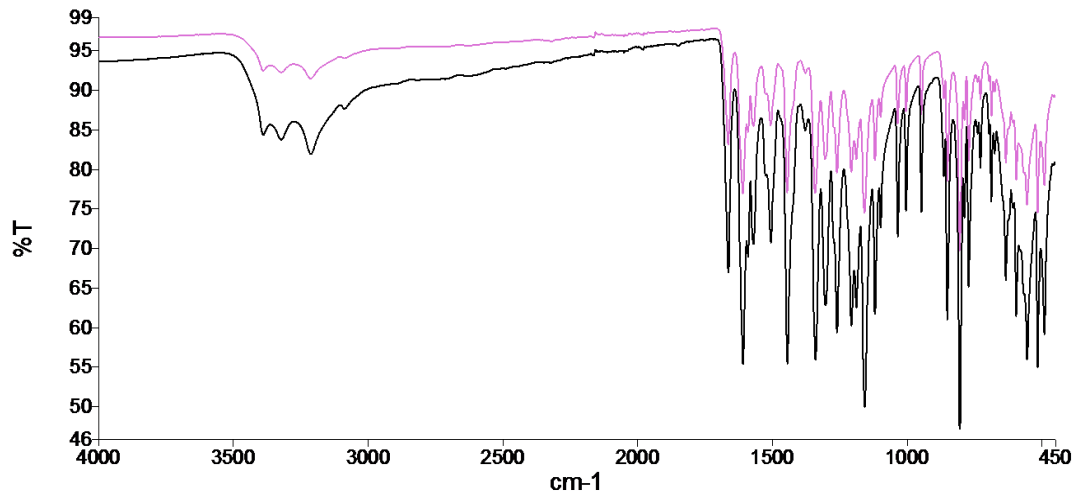

Name	Description
MML 43713639 Luteolin Canyonside UATR	11083/2022005
QC Luteolin Canyonside UATR MML 43713639	11083/2022005

## Compare Summary

Name(ID)	Best Hit	Correlation	Pass / Fail
MML 43713639 Luteolin Canyonside UATR	M:\- IDENTITY -\spectra\QC Luteolin Canyonside UATR MML 43713639.sp	0.994835	Pass

## Compare Details

Sample Name	Correlation	Pass / Fail
M:\- IDENTITY -\spectra\QC Luteolin Canyonside UATR MML 43713639.sp	0.994835	Pass

